

Instructions for Use

RealStar[®] HSV PCR Kit 1.1

11/2017 EN

RealStar[®]

HSV PCR Kit 1.1

For use with

LightCycler[®] 1.2/1.5/2.0 Instruments (Roche)



061112



48



11 2017



altona Diagnostics GmbH • Mörkenstr. 12 • D-22767 Hamburg

Content

1.	Intended Use	6
2.	Kit Components	6
3.	Storage	6
4.	Material and Devices required but not provided	7
5.	Background Information	8
6.	Product Description	8
6.1	Real-Time PCR Instruments	10
7.	Warnings and Precautions	10
8.	Procedure	11
8.1	Sample Preparation	11
8.2	Master Mix Setup	13
8.3	Reaction Setup.....	14
9.	Programming the Real-Time PCR Instrument	15
9.1	Settings	15
9.2	Fluorescence Detectors (Dyes).....	16
9.3	Temperature Profile and Dye Acquisition	16
10.	Data Analysis	17
10.1	Validity of Diagnostic Test Runs	17
10.1.1	Valid Diagnostic Test Run (qualitative).....	17
10.1.2	Invalid Diagnostic Test Run (qualitative)	17
10.1.3	Valid Diagnostic Test Run (quantitative).....	18
10.1.4	Invalid Diagnostic Test Run (quantitative).....	18
10.2	Interpretation of Results	19
10.2.1	Qualitative Analysis	19

10.2.2 Quantitative Analysis..... 19

11. Performance Evaluation 21

11.1 Analytical Sensitivity..... 21

11.2 Analytical Specificity..... 23

11.3 Linear Range..... 23

11.4 Precision 26

12. Limitations 27

13. Quality Control 28

14. Technical Assistance 28

15. Literature..... 28

16. Trademarks and Disclaimers 29

17. Explanation of Symbols 30

1. Intended Use

The RealStar® HSV PCR Kit 1.1 is an *in vitro* diagnostic test, based on real-time PCR technology, for the simultaneous detection and quantification of herpes simplex virus 1 (HSV-1) and herpes simplex virus 2 (HSV-2) specific DNA.

2. Kit Components

Lid Color	Component	Number of Vials	Volume [µl/Vial]
Blue	Master A	4	60
Purple	Master B	4	120
Green	Internal Control	1	1000
Red	HSV-1 QS1-4*	4	250
Orange	HSV-2 QS1-4*	4	250
White	Water (PCR grade)	1	500

* The RealStar® HSV PCR Kit 1.1 contains HSV-1 as well as HSV-2 Quantification Standards (QS) at four different concentrations (see Chapter 6. Product Description)

3. Storage

- The RealStar® HSV PCR Kit 1.1 is shipped on dry ice. The components of the kit should arrive frozen. If one or more components are not frozen upon receipt, or if tubes have been compromised during shipment, contact altona Diagnostics GmbH for assistance.
- All components should be stored between -25°C and -15°C upon arrival.
- Repeated thawing and freezing of Master reagents (more than twice) should be avoided, as this might affect the performance of the assay. The reagents should be frozen in aliquots, if they are to be used intermittently.
- Storage between +2°C and +8°C should not exceed a period of two hours.
- Protect Master A and Master B from light.

4. Material and Devices required but not provided

- Appropriate real-time PCR instrument (see chapter 6.1 Real-Time PCR Instruments)
- Appropriate nucleic acid extraction system or kit (see chapter 8.1 Sample Preparation)
- Desktop centrifuge with a rotor for 2 ml reaction tubes
- Vortex mixer
- LightCycler® capillaries with corresponding closing material
- Pipettes (adjustable)
- Pipette tips with filters (disposable)
- Powder-free gloves (disposable)

NOTE



Please ensure that all instruments used have been installed, calibrated, checked and maintained according to the manufacturer's instructions and recommendations.

5. Background Information

Herpes simplex virus 1 (HSV-1) and Herpes simplex virus 2 (HSV-2) are members of the family *Herpesviridae* and, along with Varicella-zoster virus (VZV), classified as *alphaherpesviridae*. HSV-1 and HSV-2 have a linear double stranded DNA genome of approximately 150 kbp. HSV-1 and HSV-2 share over 80% nucleotide identity within their protein coding region.

Herpes simplex virus infections occur worldwide with no seasonal distribution. The virus is spread by direct contact with virus in secretions. The prevalence of HSV-1 infection increases gradually from childhood, reaching 80% and more in later years, whereas the seroprevalence of HSV-2 remains low until adolescence. Most HSV-1 primary infections are acquired as subclinical or unrecognized infections. Primary infections with HSV-2 classically present as herpes genitalis. Primary infection with HSV-1 or HSV-2 is followed by the establishment of latency in the dorsal root ganglia. Periodically, the virus reactivates and travels via the nerve axon to oral or genital sites, resulting in release of infectious virus and, in some cases, lesion formation. Although usually asymptomatic, HSV infections can cause a wide spectrum of clinical manifestations, including oral herpes, genital herpes, neonatal herpes, encephalitis, and ocular herpes.

6. Product Description

The RealStar® HSV PCR Kit 1.1 is an *in vitro* diagnostic test, based on real-time PCR technology, for the simultaneous detection and quantification of herpes simplex virus 1 (HSV-1) and herpes simplex virus 2 (HSV-2) specific DNA.

The assay includes a heterologous amplification system (Internal Control) to identify possible PCR inhibition and to confirm the integrity of the reagents of the kit.

Real-time PCR technology utilizes polymerase chain reaction (PCR) for the amplification of specific target sequences and target specific probes for the detection of the amplified DNA. The probes are labelled with fluorescent reporter and quencher dyes.

Probes specific for HSV-1 DNA are labelled with a fluorophore showing similar characteristics to Cy[®]5 whereas the probes specific for HSV-2 DNA are labelled with the fluorophore FAM[™]. The probe specific for Internal Control (IC) is labelled with a fluorophore showing similar characteristics to Cy[®]3.

Using probes linked to distinguishable dyes enables the parallel detection of HSV-1 and HSV-2 specific DNA as well as the detection of the Internal Control in corresponding detector channels of the real-time PCR instrument.

The test consists of two processes in a single tube assay:

- PCR amplification of target DNA and Internal Control
- Simultaneous detection of PCR amplicons by fluorescent dye labelled probes

The RealStar® HSV PCR Kit 1.1 consists of:

- Two Master reagents (Master A and Master B)
- Internal Control (IC)
- Two sets of Quantification Standards
 - Four HSV-1 specific Quantification Standards (QS1-QS4)
 - Four HSV-2 specific Quantification Standards (QS1-QS4)
- PCR grade water

Master A and Master B contain all components (PCR buffer, DNA polymerase, magnesium salt, primers and probes) to allow PCR mediated amplification and detection of HSV-1 specific DNA, HSV-2 specific DNA and Internal Control in one reaction setup.

The Quantification Standards contain standardised concentrations of HSV-1 and HSV-2 specific DNA. The Quantification Standards can be used individually as positive controls, or together to generate a **standard curve**, which can be used to determine the concentration of HSV-1 specific DNA and/or HSV-2 specific DNA in the sample.

The Quantification Standards have the following concentrations:

Quantification Standard	Concentration [copies/μl]
QS1	1.00E+04
QS2	1.00E+03
QS3	1.00E+02
QS4	1.00E+01

6.1 Real-Time PCR Instruments

The RealStar® HSV PCR Kit 1.1 was developed and validated to be used with the following real-time PCR instruments:

- LightCycler® 1.2/1.5/2.0 Instruments (Roche)

7. Warnings and Precautions

Read the Instructions for Use carefully before using the product.

- Before first use check the product and its components for:
 - Integrity
 - Completeness with respect to number, type and filling (see chapter 2. Kit Components)
 - Correct labelling
 - Frozenness upon arrival
- Use of this product is limited to personnel specially instructed and trained in the techniques of real-time PCR and *in vitro* diagnostic procedures.
- Specimens should always be treated as infectious and/or biohazardous in accordance with safe laboratory procedures.

- Wear protective disposable powder-free gloves, a laboratory coat and eye protection when handling specimens.
- Avoid microbial and nuclease (DNase/RNase) contamination of the specimens and the components of the kit.
- Always use DNase/RNase-free disposable pipette tips with aerosol barriers.
- Always wear protective disposable powder-free gloves when handling kit components.
- Use separated and segregated working areas for (i) sample preparation, (ii) reaction setup and (iii) amplification/detection activities. The workflow in the laboratory should proceed in unidirectional manner. Always wear disposable gloves in each area and change them before entering a different area.
- Dedicate supplies and equipment to the separate working areas and do not move them from one area to another.
- Store positive and/or potentially positive material separated from all other components of the kit.
- Additional controls may be tested according to guidelines or requirements of local, state and/or federal regulations or accrediting organizations.
- Do not open the LightCycler® capillaries post amplification, to avoid contamination with amplicons.
- Do not autoclave reaction tubes after the PCR, since this will not degrade the amplified nucleic acid and will bear the risk to contaminate the laboratory area.
- Do not use components of the kit that have passed their expiration date.
- Discard sample and assay waste according to your local safety regulations.

8. Procedure

8.1 Sample Preparation

Extracted DNA is the starting material for the RealStar® HSV PCR Kit 1.1.

The quality of the extracted DNA has a profound impact on the performance of

the entire test system. It has to be ensured that the system used for nucleic acid extraction is compatible with real-time PCR technology. The following kits and systems are suitable for nucleic acid extraction:

- QIAamp® DNA Mini Kit (QIAGEN)
- QIASymphony® (QIAGEN)
- NucliSENS® easyMag® (bioMérieux)
- MagNA Pure 96 System (Roche)
- m2000sp (Abbott)
- Maxwell® 16 IVD Instrument (Promega)
- VERSANT® kPCR Molecular System SP (Siemens Healthcare)

Alternative nucleic acid extraction systems and kits might also be appropriate. The suitability of the nucleic acid extraction procedure for use with RealStar® HSV PCR Kit 1.1 has to be validated by the user.

If using a spin column based sample preparation procedure including washing buffers containing ethanol, it is highly recommended to perform an additional centrifugation step for 10 min at approximately 17000 x g (~ 13000 rpm), using a new collection tube, prior to the elution of the nucleic acid.

CAUTION



If your sample preparation system is using washing buffers containing ethanol, make sure to eliminate any traces of ethanol prior to elution of the nucleic acid. Ethanol is a strong inhibitor of real-time PCR.



The use of carrier RNA is crucial for extraction efficiency and stability of the extracted nucleic acid.

For additional information and technical support regarding pre-treatment and sample preparation please contact our Technical Support (see chapter 14. Technical Assistance).

8.2 Master Mix Setup

All reagents and samples should be thawed completely, mixed (by pipetting or gentle vortexing) and centrifuged briefly before use.

The RealStar® HSV PCR Kit 1.1 contains a heterologous Internal Control (IC), which can either be used as a PCR inhibition control or as a control of the sample preparation procedure (nucleic acid extraction) and as a PCR inhibition control.

- ▶ If the IC is used as a PCR inhibition control, but not as a control for the sample preparation procedure, set up the Master Mix according to the following pipetting scheme:

Number of Reactions (rxns)	1	12
Master A	5 µl	60 µl
Master B	10 µl	120 µl
Internal Control	1 µl	12 µl
Volume Master Mix	16 µl	192 µl

- ▶ If the IC is used as a control for the sample preparation procedure and as a PCR inhibition control, add the IC during the nucleic acid extraction procedure.
- ▶ No matter which method/system is used for nucleic acid extraction, the IC **must not** be added directly to the specimen. The IC should always be added to the specimen/lysis buffer mixture. The volume of the IC which has to be added, always and only depends on the elution volume. It represents 10% of the elution volume. For instance, if the nucleic acid is going to be eluted in 60 µl of elution buffer or water, 6 µl of IC per sample must be added into the specimen/lysis buffer mixture.

- ▶ If the IC was added during the sample preparation procedure, set up the Master Mix according to the following pipetting scheme:

Number of Reactions (rxns)	1	12
Master A	5 µl	60 µl
Master B	10 µl	120 µl
Volume Master Mix	15 µl	180 µl

CAUTION

If the IC (Internal Control) was added during the sample preparation procedure, at least the negative control must include the IC.



No matter which method/system is used for nucleic acid extraction, never add the IC directly to the specimen.

8.3 Reaction Setup

- ▶ Pipette 15 µl of the Master Mix into each required LightCycler® capillary.
- ▶ Add 10 µl of the sample (eluate from the nucleic acid extraction) or 10 µl of the controls (Quantification Standard, Positive or Negative Control).

Reaction Setup	
Master Mix	15 µl
Sample or Control	10 µl
Total Volume	25 µl

- ▶ Make sure that each Positive Control (QS) and at least one Negative Control is used per run.

- ▶ For quantification purposes all of each (HSV-1 and HSV-2) Quantification Standards (QS1 to QS4) should be used.
- ▶ Thoroughly mix the samples and controls with the Master Mix by pipetting up and down.
- ▶ Close the LightCycler® capillary with the appropriate plastic stopper.
- ▶ Centrifuge the LightCycler® capillaries using an appropriate centrifuge for 30 seconds at approximately 400 x g (~ 2000 rpm).

9. Programming the Real-Time PCR Instrument

For basic information regarding the setup and programming of the different real-time PCR instruments, please refer to the user manual of the respective instrument.

For detailed programming instructions regarding the use of the RealStar® HSV PCR Kit 1.1 on specific real-time PCR instruments please contact our Technical Support (see chapter 14. Technical Assistance).

9.1 Settings

- ▶ Define the following settings:

Settings	
Reaction Volume	25 µl*
Ramp Rate	Default

* The reaction volume has to be defined as 20 µl, if using a LightCycler® 2.0 Instrument (Roche).

9.2 Fluorescence Detectors (Dyes)

- Define the fluorescence detectors (dyes):

Target	LightCycler® 1.2/1.5	LightCycler® 2.0
HSV-2 specific DNA	F1	530
Internal Control (IC)	F2	610
HSV-1 specific DNA	F3	705

CAUTION



For accurate data analysis on the LightCycler® Instruments a specific Color Compensation File might be needed. Please contact altona Diagnostics GmbH for assistance



If using the LightCycler® 2.0 Instrument, only the detection channel 530, 610 and 705 should be activated for color compensation.

9.3 Temperature Profile and Dye Acquisition

- Define the temperature profile and dye acquisition:

	Analysis Mode	Cycle Repeats	Acquisition	Temperature [°C]	Time [min:sec]
Denaturation	None	1	-	95	02:00
Amplification	Quantification	45	None	95	00:05
			Single	60	00:30
			None	72	00:10
Cooling	None	1	-	40	00:30

10. Data Analysis

For basic information regarding data analysis on specific real-time PCR instruments, please refer to the user manual of the respective instrument.

For detailed instructions regarding the analysis of the data generated with the RealStar® HSV PCR Kit 1.1 on different real-time PCR instruments please contact our Technical Support (see chapter 14. Technical Assistance).

10.1 Validity of Diagnostic Test Runs

10.1.1 Valid Diagnostic Test Run (qualitative)

A **qualitative** diagnostic test run is **valid**, if the following control conditions are met:

Control ID	Detection Channel		
	F3/705	F1/530	F2/610
Positive Control HSV-1	+	-	+/-*
Positive Control HSV-2	-	+	+/-*
Negative Control	-	-	+

* The presence or absence of a signal in the F2/610 channel is not relevant for the validity of the test run.

10.1.2 Invalid Diagnostic Test Run (qualitative)

A **qualitative** diagnostic test run is **invalid**, (i) if the run has not been completed or (ii) if any of the control conditions for a **valid** diagnostic test run are not met.

In case of an **invalid** diagnostic test run, repeat testing by using the remaining purified nucleic acids or start from the original samples again.

10.1.3 Valid Diagnostic Test Run (quantitative)

A **quantitative** diagnostic test run is **valid**, if all control conditions for a **valid qualitative** diagnostic test run are met [see chapter 10.1.1 Valid Diagnostic Test Run (qualitative)]. The **quantification** results are **valid** if the generated **standard curve** reaches the following control parameter value:

Control Parameter	Valid Value
R square (R^2)	≥ 0.98

NOTE



Not all real-time PCR instruments display the R square (R^2) value. For detailed information, please refer to the user manual of the respective instrument.

10.1.4 Invalid Diagnostic Test Run (quantitative)

A **quantitative** diagnostic test run is **invalid**, (i) if the run has not been completed or (ii) if any of the control conditions for a **valid quantitative** diagnostic test run are not met.

In case of an **invalid** diagnostic test run, repeat testing by using the remaining purified nucleic acids or start from the original samples again.

10.2 Interpretation of Results

10.2.1 Qualitative Analysis

Detection Channel			Result Interpretation
F3/705	F1/530	F2/610	
+	-	+*	HSV-1 specific DNA detected.
-	+	+*	HSV-2 specific DNA detected.
-	-	+	Neither HSV-1 nor HSV-2 specific DNA detected. The sample does not contain detectable amounts of HSV-1 or HSV-2 specific DNA.
-	-	-	PCR inhibition or reagent failure. Repeat testing from original sample or collect and test a new sample.

* Detection of the Internal Control in the F2/610 detection channel is not required for positive results either in the F1/530 detection channel or in the F3/705 detection channel. High HSV-1 or HSV-2 DNA load/s in the sample can lead to reduced or absent Internal Control signals.

10.2.2 Quantitative Analysis

The RealStar® HSV PCR Kit 1.1 includes four Quantification Standards (QS) for HSV-1 and four Quantification Standards (QS) for HSV-2. In order to generate a **standard curve** for quantitative analysis, these have to be defined as **standards** with appropriate concentrations (see chapter 6. Product Description). Using **standards** of known concentrations a standard curve for quantitative analysis can be generated.

$$C_t = m \cdot \log(N_0) + b$$

C_t = Threshold Cycle
 m = Slope
 N_0 = Initial Concentration
 b = Intercept

Derived from the standard curve positive samples of unknown concentrations can be quantified.

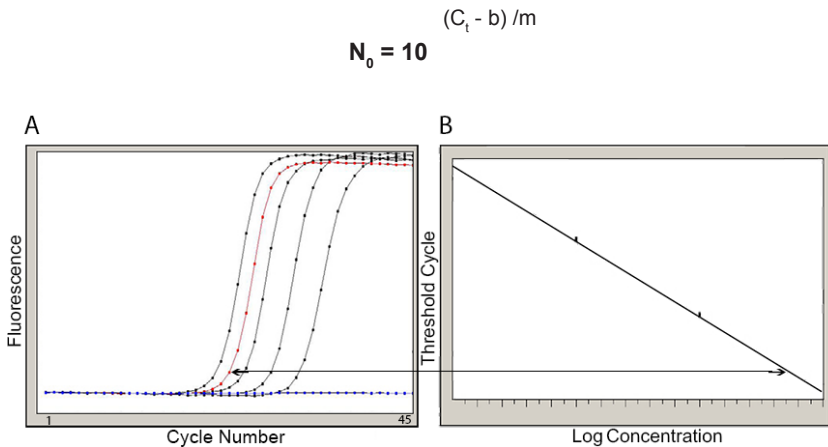


Figure 1: Quantification Standards (black), a positive (red) and a negative sample (blue) displayed in the Amplification Plot [A] and Standard Curve analysis [B]

NOTE



The concentration of the "Sample" is displayed in copies/μl and refers to the concentration in the eluate.

To determine the **viral load of the original sample**, the following formula has to be applied:

$$\text{Viral load (Sample) [copies/ml]} = \frac{\text{Volume (Eluate) } [\mu\text{l}] \cdot \text{Viral load (Eluate) [copies}/\mu\text{l}]}{\text{Sample Input [ml]}}$$

11. Performance Evaluation

Performance evaluation of the RealStar® HSV PCR Kit 1.1 was done using quantified HSV-1 specific DNA (ATCC® Number: VR-1493) and HSV-2 specific DNA (ATCC® Number: VR-540).

11.1 Analytical Sensitivity

The analytical sensitivity of the RealStar® HSV PCR Kit 1.1 is defined as the concentration (copies/ μl of the eluate) of HSV-1 or HSV-2 specific DNA molecules that can be detected with a positivity rate of 95%. The analytical sensitivity was determined by analysis of dilution series of quantified HSV-1 DNA and HSV-2 DNA.

Table 1: PCR results used for the calculation of the analytical sensitivity with respect to the detection of HSV-1 specific DNA

Input Conc. [copies/ μl]	Number of Replicates	Number of Positives	Hit Rate [%]
3.162	12	12	100
1.000	12	12	100
0.316	12	12	100
0.200	12	11	92
0.100	12	5	42
0.032	12	3	25
0.010	12	2	17
0.003	12	0	0
0.001	12	0	0

Table 2: PCR results used for the calculation of the analytical sensitivity with respect to the detection of HSV-2 specific DNA

Input Conc. [copies/μl]	Number of Replicates	Number of Positives	Hit Rate [%]
3.162	12	12	100
1.000	12	12	100
0.316	12	12	100
0.200	12	8	67
0.100	11	5	45
0.032	12	0	0
0.010	12	1	8
0.003	12	0	0
0.001	12	0	0

The analytical sensitivity of the RealStar® HSV PCR Kit 1.1 was determined by Probit analysis:

- For the detection of HSV-1 specific DNA, the analytical sensitivity is 0.41 copies/μl eluate [95% confidence interval (CI): 0.23 - 1.20 copies/μl]
- For the detection of HSV-2 specific DNA, the analytical sensitivity is 0.50 copies/μl eluate [95% confidence interval (CI): 0.29 - 1.41 copies/μl]

11.2 Analytical Specificity

The analytical specificity of the RealStar® HSV PCR Kit 1.1 is ensured by the thorough selection of the oligonucleotides (primers and probes). The oligonucleotides were checked by sequence comparison analysis against publicly available sequences to ensure that all relevant herpes simplex virus 1 and 2 genotypes will be detected.


The RealStar® HSV PCR Kit 1.1 did not cross-react with any of the following pathogens:

- BK virus
- Cytomegalovirus
- Epstein-Barr virus
- Hepatitis B virus
- Hepatitis C virus
- Human herpesvirus 6A
- Human herpesvirus 6B
- Human herpesvirus 7
- Human herpesvirus 8
- Human immunodeficiency virus 1
- Human parvovirus B19
- JC virus
- Varicella-zoster virus

11.3 Linear Range

The linear range of the RealStar® HSV PCR Kit 1.1 was evaluated by analysing a logarithmic dilution series of HSV-1 and HSV-2 specific DNA using concentrations ranging from 1E+08 to 1E+00 copies/µl. At least three replicates per dilution were analysed.

A

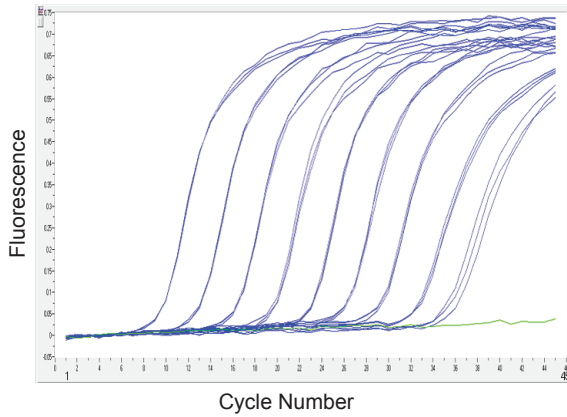

B

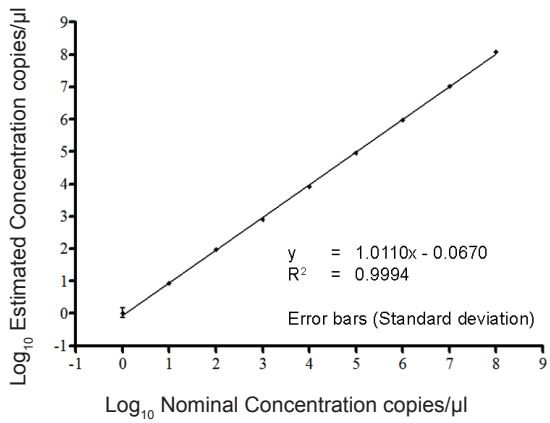


Figure 2: Amplification curves **[A]** and linear regression **[B]** of an analysed dilution series of HSV-1 specific DNA

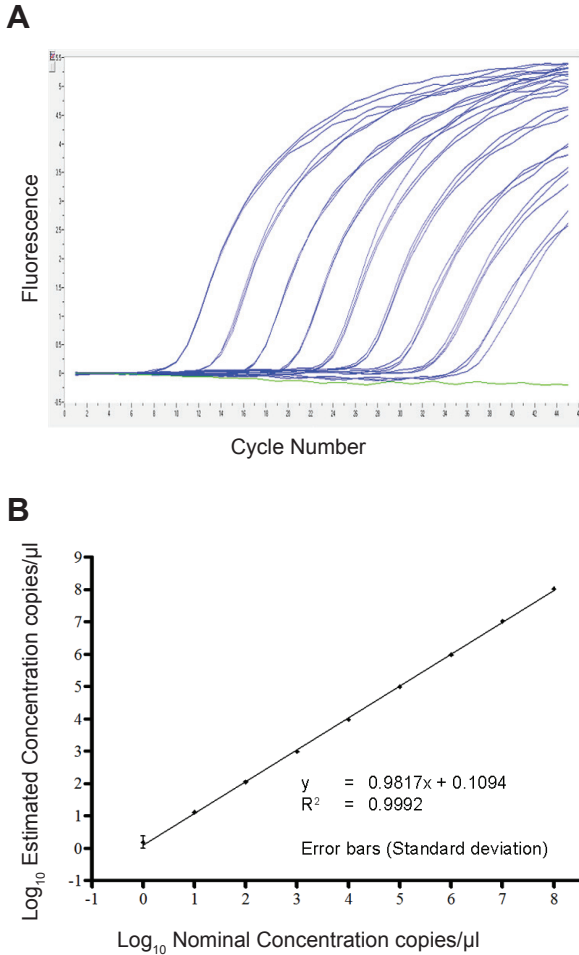


Figure 3: Amplification curves **[A]** and linear regression **[B]** of an analysed dilution series of HSV-2 specific DNA

The linear range of the RealStar® HSV PCR Kit 1.1 for HSV-1 specific DNA extends over an interval of at least **eight** orders of magnitude and for HSV-2 specific DNA over an interval of at least **eight** orders of magnitude.

11.4 Precision

Precision of the RealStar® HSV PCR Kit 1.1 was determined as intra-assay variability (variability within one experiment), inter-assay variability (variability between different experiments) and inter-lot variability (variability between different production lots). Total variability was calculated by combining the three analyses.

Variability data are expressed in terms of standard deviation and coefficient of variation. The data are based on quantification analysis of defined concentrations of HSV-1 and HSV-2 specific DNA and on threshold cycle (C_t) value in terms of the Internal Control. At least six replicates per sample were analysed for intra-assay, inter-assay and inter-lot variability.

Table 3: Precision data for the detection of HSV-1 and HSV-2 specific DNA

HSV-1 and HSV-2		Average Conc. [copies/ μ l]	Standard Deviation	Coefficient of Variation [%]
Intra-Assay Variability	HSV-1	142.36	5.98	4.20
	HSV-2	160.01	8.19	5.12
Inter-Assay Variability	HSV-1	147.76	8.28	5.60
	HSV-2	161.78	11.05	6.83
Inter-Lot Variability	HSV-1	142.07	7.36	5.18
	HSV-2	160.96	10.37	6.44
Total Variability	HSV-1	145.76	8.79	6.03
	HSV-2	161.82	11.34	7.01

Table 4: Precision data for the detection of the Internal Control

Internal Control	Average Threshold Cycle (C _t)	Standard Deviation	Coefficient of Variation [%]
Intra-Assay Variability	26.16	0.04	0.13
Inter-Assay Variability	26.12	0.05	0.19
Inter-Lot Variability	26.10	0.05	0.17
Total Variability	26.12	0.05	0.19

12. Limitations

- Strict compliance with the Instructions for Use is required for optimal results.
- Use of this product is limited to personnel specially instructed and trained in the techniques of real-time PCR and *in vitro* diagnostic procedures.
- Good laboratory practice is essential for proper performance of this assay. Extreme care should be taken to preserve the purity of the components of the kit and reaction setups. All reagents should be closely monitored for impurity and contamination. Any suspicious reagents should be discarded.
- Appropriate specimen collection, transport, storage and processing procedures are required for the optimal performance of this test.
- This assay must not be used on the specimen directly. Appropriate nucleic acid extraction methods have to be conducted prior to using this assay.
- The presence of PCR inhibitors (e.g. heparin) may cause underquantification, false negative or invalid results.
- Potential mutations within the target regions of the HSV-1 and HSV-2 genome covered by the primers and/or probes used in the kit may result in underquantification and/or failure to detect the presence of the pathogens.
- As with any diagnostic test, results of the RealStar® HSV PCR Kit 1.1 need to be interpreted in consideration of all clinical and laboratory findings.

13. Quality Control

In accordance with the Altona Diagnostics GmbH EN ISO 13485-certified Quality Management System, each lot of RealStar® HSV PCR Kit 1.1 is tested against predetermined specifications to ensure consistent product quality.

14. Technical Assistance

For technical advice, please contact our Technical Support:

e-mail: **support@altona-diagnostics.com**
phone: **+49-(0)40-5480676-0**

15. Literature

Versalovic, James, Carroll, Karen C., Funke, Guido, Jorgensen, James H., Landry, Marie Louise and David W. Warnock (ed). Manual of Clinical Microbiology. 10th Edition. ASM Press, 2011.

Cohen, Jonathan, Powderly, William G, and Steven M Opal. Infectious Diseases, Third Edition. Mosby, 2010.

16. Trademarks and Disclaimers

RealStar® (altona Diagnostics); ABI Prism® (Applied Biosystems); ATCC® (American Type Culture Collection); CFX96™ (Bio-Rad); Cy® (GE Healthcare); FAM™, JOE™, ROX™ (Life Technologies); LightCycler® (Roche); SmartCycler® (Cepheid); Maxwell® (Promega); Mx 3005P™ (Stratagene); NucliSENS®, easyMag® (bioMérieux); Rotor-Gene®, QIAamp®, MinElute®, QIASymphony® (QIAGEN); VERSANT® (Siemens Healthcare).

Registered names, trademarks, etc. used in this document, even if not specifically marked as such, are not to be considered unprotected by law.

















The RealStar® HSV PCR Kit 1.1 is a CE-marked diagnostic kit according to the European *in vitro* diagnostic directive 98/79/EC.

Product not licensed with Health Canada and not FDA cleared or approved.

Not available in all countries.

© 2017 altona Diagnostics GmbH; all rights reserved.

17. Explanation of Symbols

Symbol	Explanation
	<i>In vitro</i> diagnostic medical device
	Batch code
	Cap color
	Product number
	Content
	Number
	Component
	Global trade identification number
	Consult instructions for use
	Contains sufficient for “n” tests/reactions (rxns)
	Temperature limit
	Use-by date
	Manufacturer
	Caution
	Notes
	Version

always a drop ahead.

altona Diagnostics GmbH
Mörkenstr. 12
22767 Hamburg, Germany

phone +49 40 548 0676 0
fax +49 40 548 0676 10
e-mail info@altona-diagnostics.com

www.altona-diagnostics.com

